

**This item is the archived peer-reviewed author-version of:**

Analysis of short-lived reactive species in plasma-air-water systems : the dos and the do nots

**Reference:**

Gorbanev Yury, Privat-Maldonado Angela, Bogaerts Annemie.- Analysis of short-lived reactive species in plasma-air-water systems : the dos and the do nots  
Analytical chemistry - ISSN 0003-2700 - 90:22(2018), p. 13151-13158  
Full text (Publisher's DOI): <https://doi.org/10.1021/ACS.ANALCHEM.8B03336>  
To cite this reference: <https://hdl.handle.net/10067/1563010151162165141>

## Analysis of short-lived reactive species in plasma-air-water systems: The do's and the don'ts

Yury Gorbanev, Angela Privat-Maldonado, and Annemie Bogaerts

*Anal. Chem.*, **Just Accepted Manuscript** • DOI: 10.1021/acs.analchem.8b03336 • Publication Date (Web): 05 Oct 2018

Downloaded from <http://pubs.acs.org> on October 7, 2018

### Just Accepted

“Just Accepted” manuscripts have been peer-reviewed and accepted for publication. They are posted online prior to technical editing, formatting for publication and author proofing. The American Chemical Society provides “Just Accepted” as a service to the research community to expedite the dissemination of scientific material as soon as possible after acceptance. “Just Accepted” manuscripts appear in full in PDF format accompanied by an HTML abstract. “Just Accepted” manuscripts have been fully peer reviewed, but should not be considered the official version of record. They are citable by the Digital Object Identifier (DOI®). “Just Accepted” is an optional service offered to authors. Therefore, the “Just Accepted” Web site may not include all articles that will be published in the journal. After a manuscript is technically edited and formatted, it will be removed from the “Just Accepted” Web site and published as an ASAP article. Note that technical editing may introduce minor changes to the manuscript text and/or graphics which could affect content, and all legal disclaimers and ethical guidelines that apply to the journal pertain. ACS cannot be held responsible for errors or consequences arising from the use of information contained in these “Just Accepted” manuscripts.



# Analysis of short-lived reactive species in plasma-air-water systems: The do's and the don'ts

Yury Gorbanev\*,<sup>1</sup> Angela Privat-Maldonado,<sup>1,2</sup> Annemie Bogaerts<sup>1</sup>

<sup>1</sup>Research group PLASMANT, Department of Chemistry, University of Antwerp, Wilrijk, Antwerpen, Belgium BE-2610

<sup>2</sup>Center for Oncological Research (CORE), University of Antwerp, Wilrijk, Antwerpen, Belgium BE-2610

This Feature Article addresses the analysis of the reactive species generated by non-thermal atmospheric pressure plasmas, which are widely employed in industrial and biomedical research, as well as first clinical applications. We summarise the progress in detection of plasma-generated short-lived reactive oxygen and nitrogen species in aqueous solutions, discuss the potential and limitations of various analytical methods in plasma-liquid systems, and provides an outlook on the possible future research goals in development of short-lived reactive species analysis methods for a general non-specialist audience.

## 1. Cold atmospheric pressure plasmas: research and applications, reactive species, and interaction with liquids.

Plasma is an ionised gas, often (controversially<sup>1</sup>) referred to as the fourth state of matter. It contains neutral gas molecules and atoms, but also electrons and various types of ions, excited species and radicals. Plasmas are generally divided into several types based on the operating temperature and pressure. First, we can distinguish (i) high-temperature plasmas, operating at temperatures of (several) million K (as used for fusion research, mimicking the conditions of the Sun) and (ii) low temperature plasmas. The latter can still be subdivided into thermal plasmas, operating at temperatures of a few thousand K (such as inductively coupled plasma used for ICP-MS and ICP-OES in analytical chemistry), and non-thermal plasmas, where the gas remains at room temperature (and up to 1000 K) but the electrons are heated to 10,000 – 30,000 K (1-3 eV). These non-thermal ('cold') plasmas are also called 'gas discharges',<sup>2</sup> and operate at either low pressure (e.g., glow discharges used for GDMS and GD-OES in analytical chemistry) or atmospheric pressure (e.g., plasma jets and dielectric barrier discharges, also used as ion sources in analytical chemistry for ambient ionization mass spectrometry).<sup>3,4</sup>

These cold atmospheric pressure plasmas (CAPs) are not only important in analytical chemistry, but they have gained significant interest in recent years due to their unique properties. They can be generated by applying an electric field to a gaseous medium at ambient pressure and near-ambient ('low' compared to thermal plasmas) temperature.<sup>5,6</sup>

CAPs produce various reactive oxygen and nitrogen species (RONS) which define their potential applications<sup>5,7</sup> (Fig. 1). The applications include photoresist removal,<sup>8</sup> plasma catalysis,<sup>9,10</sup> thin

film deposition and modification,<sup>5,11</sup> production of enhanced nano-materials,<sup>12</sup> plasma-assisted polymerisation,<sup>5,13</sup> waste water treatment,<sup>11,14</sup> removal of volatile organic chemicals from air,<sup>10,15</sup> conversion of CO<sub>2</sub> into value-added chemicals,<sup>16</sup> etc.

Moreover, cold plasma is a valuable tool in chemical synthesis.<sup>17,18</sup> Being able to efficiently initiate radical chain reactions in systems comprised of gaseous plasma and liquids,<sup>18</sup> CAP is an attractive alternative to conventional radical initiators.

However, the most burgeoning field of CAP research is biomedical and agricultural applications. The agricultural utilisations of CAPs are enhancement of seed germination, anti-bacterial and anti-fungal treatment of plants,<sup>19</sup> similarly to food processing, which makes use of the decontaminating properties of cold plasma.<sup>20</sup> The vast area of CAP applications in biomedicine spreads from dentistry (teeth whitening, disinfection)<sup>21,22</sup> and production of surfaces with anti-bacterial resistance<sup>23</sup> to various sterilisations processes,<sup>24,25</sup> wound healing,<sup>24</sup> deactivation of bacteria and viruses,<sup>26,27</sup> but the field that recently attracts most attention is cancer treatment.<sup>24,28-30</sup> In many cases, biomedical CAPs are plasma jets in which plasma is created with a noble gas (Ar<sup>30</sup> or He<sup>27,28</sup>), although air is also used.<sup>31</sup>

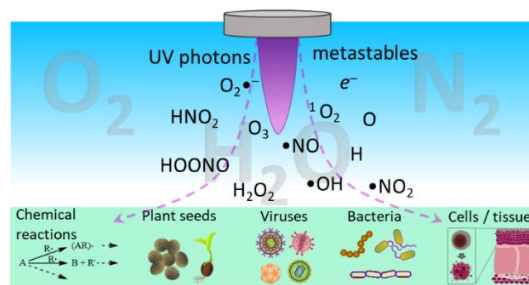


Figure 1. Cold plasma in contact with liquids produces various RONS for diverse chemical, agricultural and medical applications.

The reactive species are created either within the plasma<sup>32</sup> (e.g., using He with O<sub>2</sub> admixture<sup>28</sup>), or upon its interaction with the surrounding atmosphere<sup>30,33</sup> (N<sub>2</sub>, O<sub>2</sub>, and H<sub>2</sub>O vapour in air).

The reactive species are created either within the plasma<sup>32</sup> (e.g., using He with O<sub>2</sub> admixture<sup>28</sup>), or upon its interaction with the surrounding atmosphere<sup>30,33</sup> (N<sub>2</sub>, O<sub>2</sub>, and H<sub>2</sub>O vapour in air). The resulting RONS 'cocktail' consists of various atomic, radical, ionic and molecular species, such as O, O<sub>3</sub>, <sup>1</sup>O<sub>2</sub>, •OH,

$O_2\bullet^-$ ,  $\bullet OOH$ ,  $\bullet NO$ ,  $ONOO^-$  and  $OONO^-$ ,  $H_2O_2$ ,  $NO_2^-$ ,  $NO_3^-$ . These species, when interacting with biological substrates, are responsible for the plasma-elicited effects.<sup>7,24,30</sup> Their analysis, both qualitative ('Is this species present in a particular plasma system?') and quantitative ('At what concentrations?'), is paramount for understanding and tailoring the desired effects of CAP.<sup>34,35</sup>

The gas phase plasma does not interact with dry biological substrates: water plays an essential role in food processing, agricultural and – especially - biological milieu. The primary RONS, such as  $\bullet OH$ ,  $\bullet NO$ ,  $H_2O_2$ ,  $O$ ,  $O_3$ , are mainly created in the gas phase plasma<sup>7,32,33</sup> and undergo transformations in the liquid, although in certain cases (i.e., plasma discharge to the liquid surface) they can be created in the interface layer of aqueous solutions.<sup>30,35</sup> Secondary RONS, such as e.g.  $\bullet OH$  and  $\bullet NO_2$  from  $HOONO$ ,  $HNO_2$  and  $HNO_3$  from  $\bullet NO$  and  $\bullet NO_2$ , are the result of degradation or interaction of the primary RONS with each other or molecules in media.<sup>7,36</sup>

Chemical modelling together with various analytical techniques (e.g., optical spectroscopy and mass spectrometry methods) aids in studying the composition of the gas phase plasma<sup>7,32,37</sup> Recently, efforts in computational chemistry have addressed the interaction of gas phase RONS with aqueous solutions.<sup>37-39</sup> However, experimental monitoring of RONS in liquid is crucial for model benchmarking, and provides the most direct information on the reactive species present in the liquid.

This Feature Article focusses on the short-lived reactive species induced by CAP in aqueous solutions, and methods of their detection, identification and quantification.

The information on the identified limitations of the methods is also important for the generalist audience dealing with the detection of short-lived RONS in solutions, in systems different from CAPs.

## 2. Which RONS? Two types of plasma application mode.

The species potentially present in the analyte solutions depend on the actual CAP application mode. One option is a pre-treatment of a relevant liquid medium by CAP, with further application to a biological target.<sup>24,27,28,30</sup> In this so-called indirect treatment, the effects of plasma are attributed to long-lived molecular and ionic chemical species, which remain in solution after CAP treatment, such as  $H_2O_2$ ,  $NO_2^-$ ,  $NO_3^-$ <sup>30,40</sup> (Fig. 2). Spectrophotometry is most commonly employed to detect and quantify these species.<sup>41</sup> For example,  $H_2O_2$  is often measured using colourimetry with titanium(IV) oxalate or vanadate solutions.<sup>27,30</sup> The colourimetric detection of the nitrate/nitrite pair uses Griess reagent, and is not influenced by other long-lived plasma RONS.<sup>42</sup> Many of these detection methods are described in the recent paper by Massima Mouelet al.,<sup>41</sup> albeit without selectivity discussion.

The second application mode involves direct CAP treatment of the biological target (e.g., bacterial or cancer cells in a liquid medi-

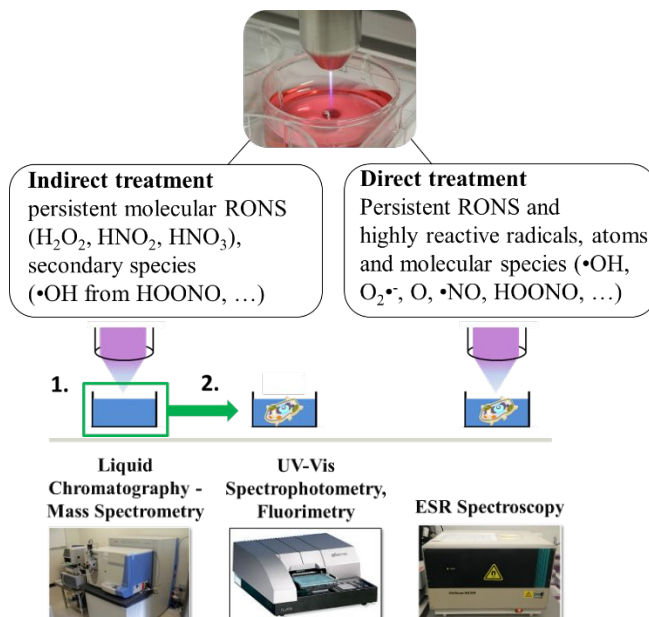


Figure 2. Two methods of plasma application, RONS in solutions and main analytical techniques used for their detection.

um).<sup>24,27</sup> Here, the RONS mixture does not only contain persistent

RONS, but also the short-lived radical and atomic species:  $O$ ,  $\bullet NO$ ,  $\bullet OH$ ,  $O_2\bullet^-$ ,  $\bullet OOH$ , as well as non-radical chemical compounds, such as singlet oxygen  $^1O_2$ . These species have diverse effects, from direct oxidative stress<sup>7</sup> to regulation of various cellular processes.<sup>43</sup>

Importantly, they were shown to play a critical role in bacterial inactivation,<sup>44</sup> cancer cell apoptosis<sup>45</sup> and immunogenic cell death,<sup>46</sup> and were suggested to be the major effectors in the degradation of organic compounds in water.<sup>47</sup> Therefore, their analysis in liquid in contact with plasma is of immense importance for the deconvolution of plasma chemistry and effects.<sup>35</sup>

Similarly to the long-lived RONS, the short-lived ones are also often measured using spectrophotometric methods.<sup>41,48</sup> However, colourimetric and fluorometric systems consisting of complex organic molecules, and based on either decay or induction of colour or fluorescence, lack selectivity (see detailed discussion in section 3).

Other reported analytical methods include liquid chromatography coupled with mass spectrometry (LC-MS) of the RONS-modified chemical substrates, and electron spin resonance (ESR) spectroscopy.<sup>27,32,33,44</sup>

In plasma-liquid systems, the selectivity of analysis becomes detrimental: plasma generates many different RONS, which are delivered to the liquid at the same time. The other problem arises from the analysis being only semi-quantitative in most cases. In the following section, we discuss the main three analytical methods used for the analysis of plasma-air-water systems in terms of these problems.

## 3. Analysis of short-lived RONS.

### 3.1. Optical spectroscopic analysis of plasma-induced RONS.

Optical spectroscopic methods are probably the most widely-used methods for the detection of short-lived RONS via

modification of substrates, both historically and based on the equipment availability. Some of them used in plasma-liquid research are described in the recent review by Massima Mouele et al.<sup>41</sup>

Many of the chemical reactions used in these methods were adapted by the plasma community from known analyses in biological milieu, and are sometimes used disregarding the limitations. Here, we present a general description of the methods with several examples, to show some selectivity-based limitations.

Spectroscopic methods comprise UV-Vis spectrophotometry and fluorimetry (measurements of the intensity of induced or reduced colour, or induced fluorescence upon reactions of chemical probes with the plasma-produced RONS in liquids), and direct UV spectrophotometry. The latter technique was used to detect ONOO<sup>-</sup> based on its characteristic absorption, although high-pH medium is required to stabilise ONOO<sup>-</sup> for subsequent UV analysis.<sup>49</sup>

Coloured dyes are degraded by CAP-induced RONS, and the loss of colour can be quantified using UV-Vis spectrophotometry.<sup>50</sup> Some of the most commonly used dyes used to assess ROS are methylene blue and methylene red,<sup>47,51</sup> which are often used in research of CAP for removal of pollutants during waste water treatment.

The main disadvantage of this method is the non-specific degradation of such dyes. For instance, decolouration of methylene blue can be a result of reactions with •OH, O, and O<sub>3</sub>.<sup>52</sup> O<sub>2</sub>•<sup>-</sup> can also be detected by degradation of dyes<sup>53</sup> with similar selectivity issues. For example, the induction of chemiluminescence ascribed to the presence of •OH and O<sub>2</sub>•<sup>-</sup> (i.e., non-selectively) was observed at the CAP-liquid interface when alkaline solutions of luminol were exposed to plasma.<sup>54</sup>

Similarly, induction of fluorescent properties of chemical molecules is also used.<sup>55,56</sup> Terephthalic acid (TA) is very often used to detect •OH in CAP-liquid systems.<sup>57,58</sup> The method is based on the induced fluorescence due to the formation of hydroxy-substituted TA. However, possible degradation of TA by plasma species (e.g. combination of O<sub>3</sub>, •OH, H<sub>2</sub>O<sub>2</sub> and UV photons<sup>59</sup>) is usually not taken into account.

Thus, optical spectroscopy methods can be used for both qualitative and semi-quantitative, albeit in most cases very non-selective, detection of the plasma-induced RONS in liquids. The advantage of the method is the possible direct visualisation requiring no equipment for a qualitative analysis a simple 'present/not present' and 'less/more' assessment can be done by naked eye.<sup>54</sup> An interesting and important use of colourimetry and fluorimetry is introducing respective chemical probes in aqueous compartments of a gel to investigate the depth of the RONS penetration into the gel as a tissue model.<sup>60</sup>

### 3.2. ESR analysis.


ESR is the most direct method of radical detection in liquid systems. It is used for the detection of paramagnetic compounds in general, and free radicals (systems with unpaired electrons) specifically.<sup>61</sup>

In most cases, free radicals are too short-lived to be detected directly. A technique of 'trapping' radicals by reacting them with

organic molecules, usually nitrones, is therefore used.<sup>62</sup> Spin traps undergo addition reactions with radicals, yielding more persistent radical adducts, which can be monitored by ESR within reasonable timescales (min to h).<sup>41,63</sup>

Another method is using a spin probe: usually a hydroxylamine of a stable nitroxide.<sup>64</sup> Upon reaction with RONS, a stable nitroxide is formed via the abstraction of an H atom from the hydroxylamine group, and the concentration of this nitroxide radical is measured. Both methods are illustrated in Scheme 1.

These two methods of radical detection are frequently used in biological milieu, both in liquid media and intracellularly.<sup>65</sup> They have been adopted by the plasma community in the last decade, and since then widely employed in cold plasma-liquid systems, where they are used to detect •OH<sup>66-68</sup> and O<sub>2</sub>•<sup>-</sup>,<sup>66,68</sup> NO•,<sup>69,70</sup> O and O<sub>3</sub>,<sup>27,33,71</sup> and <sup>1</sup>O<sub>2</sub>.<sup>27,66</sup> Extensive ESR detection studies covering many of the biologically-relevant CAP-induced RONS in aqueous solutions were performed.<sup>70,72</sup> We have previously used spin trapping of the radicals produced from isotopically labelled water to investigate the sources (vapour or liquid) of RONS induced in treated solutions.<sup>32,33,73</sup> Spin trapping was also used to monitor radicals produced from organic solvents in a polymeric solution treated by CAP,<sup>12</sup> and in water-alcohol mixtures.<sup>74</sup>

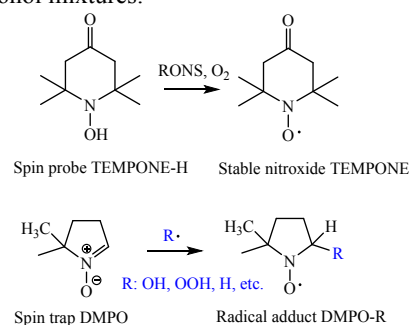

**Scheme 1. Formation of ESR-detectable nitroxide radicals from the spin probe 1-hydroxy-2,2,6,6-tetramethyl-4-oxo-piperidine (TEMPONE-H) and the spin trap 5,5-dimethyl-1-pyrroline N-oxide (DMPO).**

However, there are both general and specific limitations associated with ESR detection of radicals via spin trapping which are sometimes ignored, or otherwise unknown, in the community. We will try to address them here.

1) First, the detection of radicals by ESR (not limited to plasma-liquid systems) is seldom quantitative. The concentrations of the radical adducts or nitroxides from hydroxylamines are easily obtained using calibration with solutions of stable radicals (e.g. 2,2,6,6-tetramethylpiperidine (TEMPO) or similar stable nitroxides) of known concentration.<sup>32,33,70</sup> However, these values represent only a fraction of the total amount of radicals entering the liquid, which surprisingly is sometimes overlooked.<sup>67</sup> Free radicals undergo various reactions: recombination (•OH to H<sub>2</sub>O<sub>2</sub>), side reactions with water molecules (•NO, •NO<sub>2</sub>), reactions with organic components of the media and other scavengers,<sup>18,27,70</sup> etc. This limits the amount of the trapped radicals based on specific reaction rates. Nevertheless, the changes of these trapped amounts correspond to the changes of the total concentration of radicals (or atoms),<sup>33,71</sup> so qualitative trends can be revealed and yield useful information.

2) The second limitation is the non-selectivity of spin probes and spin traps. However, these two types of ESR 'reagents' require rather different selectivity-related considerations, as we demonstrate with several examples.




In a recent study, TEMPONE-H (see Scheme 1) was used to detect  $O_2^{\bullet-}$ ,  $\bullet NO$ , and peroxynitrite  $ONOO^-$  (short-lived at physiological pH),<sup>75,76</sup> due to its high affinity towards these species. However,

TEMPONE-H also reacts with  $\bullet OH$ .<sup>77</sup> Moreover, hydroxylamines of stable nitroxides are easily oxidised, even by  $O_2$  from air,<sup>69,78</sup> and thus also by  $O_3$ ,  $O$ , and other ROS produced by plasma. This, once again, is a general difference between biological systems (where only e.g.  $ONOO^-$  and  $O_2^{\bullet-}$  are produced by biological bodies in vitro<sup>56,79</sup>) and plasma-air-liquid systems, where a much larger variety of RONS is delivered into the liquid at the same time.

The non-selectivity of spin trapping, on the other hand, is a useful property rather than a disadvantage, because many radicals can be identified simultaneously from the same spectrum. For example, spin trap 5,5-dimethyl-1-pyrroline *N*-oxide (DMPO) forms relatively stable radical adducts with  $\bullet OH$  and  $H$ .<sup>33</sup> In a mixture of radical adducts, each adduct has a unique spectral pattern, due to different hyperfine values defined by the interactions of an unpaired electron with nearby nuclei. In other words, DMPO-OH is distinguishable from e.g. DMPO-H due to different hyperfine values, using ESR simulations.<sup>32,33</sup>

In certain cases, however, this non-selectivity can produce false-positive results, and needs to be taken into account when performing spin trapping experiments. One of the important cases is spin trapping of the CAP-produced  $\bullet NO$ . In CAP-liquid systems, delivery of both  $\bullet NO$  radicals and  $HNO_2$  to the liquid is feasible. A spin trap comprising a complex of *N*-methyl-D-glucamine dithiocarbamate (MGD) with iron(II) ion forms  $(MGD)_2Fe^{2+}$ -NO radical adducts, both with  $\bullet NO$  and  $NO_2^-$  (Scheme 2).<sup>80</sup>

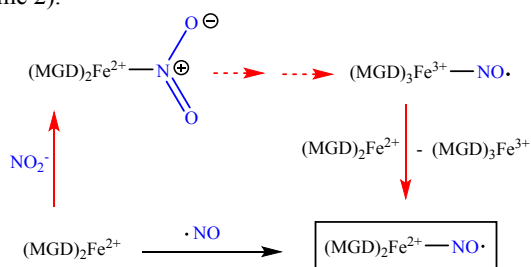

**Scheme 2. Formation of the NO adduct in reactions of *N*-methyl-D-glucamine dithiocarbamate (MGD)-iron(II) complex with nitric oxide and nitrite anion. Side reactions leading to the adduct are marked with red arrows.**

Similarly, DMPO-OH can be formed as a result of a nucleophilic attack of  $H_2O$  molecules on a carbon atom of the  $C=N$  bond in DMPO.<sup>81,82</sup> In these cases, control experiments with no radical production by plasma<sup>69</sup> are required to evaluate the contribution of the side reactions leading to false-positive results (i.e., not from direct spin trapping).

Another example is the oxidation of 2,2,6,6-tetramethylpiperidine (TEMP) or other cyclic amines to the respective stable nitroxides. Directly adapted from biological systems,<sup>83</sup> this reaction has been used to detect  $^1O_2$  in water exposed to CAP.<sup>66,70,72</sup> However, unlike those systems, cold plasma produces other RONS, which can oxidise TEMP. Takamatsu et al. used  $NaN_3$  as a specific quencher for  $^1O_2$  to evaluate its contribution to the formation of the nitroxide radical.<sup>72</sup> Note however that while this method is suitable for

media with physiological pH,  $NaN_3$  also reacts with  $O_3$  under basic conditions.<sup>84</sup> In our previous work we showed that besides  $^1O_2$ , the only other plasma-induced RONS that can oxidise TEMP are  $O_3$  and  $O$ .<sup>33</sup> By comparing the densities of  $O_3$  and  $O$  in the gas plasma with the trends of TEMPO formation in the liquid, the main contributor to this oxidation can be determined.<sup>71</sup> This, however, would be specific to each particular plasma-liquid system.

It is worth mentioning that the (non-)selectivity feature can sometimes be an artifact of a spin adduct degradation. For example, the stability of DMPO-OOH radical adduct is low, and the adduct readily transforms into DMPO-OH.<sup>85,86</sup> In such cases, using a scavenger to eliminate one of the possible contributors to the final adduct formation may be required. As an example, superoxide dismutase can be used to estimate the contributions of  $\bullet OH$  and  $O_2^{\bullet-}$  on the detected DMPO-OH.<sup>66</sup>

This brings us to the next limitation, inherent to ESR in liquids treated by CAPs.


3) The third limitation is the degradation of nitroxides in plasma-liquid systems. Both spin traps and spin adducts are organic molecules, and as such are prone to degradation by plasma-induced RONS. It was suggested that organic pollutants (and model dye molecules) are degraded in plasma-treated liquids by  $\bullet OH$  radicals,  $O$  or  $O_3$ , and solvated electrons from plasma.<sup>14,47,87,88</sup> Similar pathways are possible for spin traps and adducts. Indeed, the spin trap 5-(diethoxyphosphoryl)-5-methyl-1-pyrroline *N*-oxide (DEPMPO) was shown to degrade and form a detectable carbon-centred radical in aqueous solutions upon plasma treatment.<sup>33</sup> *N*-tert-butyl- $\alpha$ -phenylnitron (PBN) can undergo degradation to *tert*-butyl hydronitroxide upon reactions with  $\bullet OH$ .<sup>89</sup> DMPO is non-selectively oxidised to 5,5-dimethyl-2-pyrrolidone *N*-oxyl (DMPOX) by e.g.  $^1O_2$ <sup>90</sup> or media-derived oxidants such as hypochlorite.<sup>91,92</sup> In many cases, this does not present a problem due to a large excess of unreacted spin trap. However, in plasma-liquid systems, and especially in systems when plasma is ignited without gas flow,<sup>46,93</sup> mass transfer within the liquid may be limited.<sup>35</sup> This can result in only the top layer of solution reacting with RONS. In this case, the degradation of the spin trap and/or spin adduct may dominate, resulting in a decrease of the obtained ESR signal. It is therefore important to study the development of the adduct concentration within the experimental timeframe.<sup>32,33,71</sup>

Spin adducts are only relatively stable, and undergo decay over extended periods of time.<sup>61,65</sup> Thus, standardisation of experimental procedures (i.e., time between plasma exposure and ESR measurements) is necessary to obtain any reliable information.

Regarding the CAP-water systems, spin adducts also react with various CAP-induced radicals as well as  $O$  and/or  $O_3$ , yielding non-paramagnetic compounds (Scheme 3). This was demonstrated in plasma-treated water for stable nitroxide TEMPO and a PBN- $^2H$  radical adducts, which decayed with similar rates, suggesting similar decay pathways.<sup>69</sup> The reactions of the nitroxide group with  $\bullet OH$ ,  $H$ ,  $O_3/O$ , and other plasma-induced RONS may lead to complete loss of the ESR signal, and thus affect even the semi-quantitative results.<sup>69,94,95</sup>

Using an excess of the spin trap to avoid the loss of the signal upon decay becomes impractical when the spin trap itself is a radical: the ESR signal of the product will be dwarfed by the signal of the spin trap. This can be demonstrated with 2-phenyl-

4,4,5,5-tetramethylimidazoline 1-oxyl-3-oxide (PTIO) spin trap or its derivatives, which are used to detect  $\bullet\text{NO}$  in CAP-exposed solutions.<sup>56,72</sup> PTIO reacts with  $\bullet\text{NO}$  to produce 2-phenyl-4,4,5,5-tetramethylimidazoline 1-oxyl (PTI)<sup>96</sup> as shown in Scheme 5. Since both PTIO and PTI are nitroxides, they lose their radical nature in CAP-treated water due to reactions with plasma-induced RONS (see Scheme 3). Moreover, PTI can be oxidised back to PTIO by plasma-induced ROS (Scheme 4). As a result, the decay rate of the product (PTI) may even exceed that of the reagent (PTIO).<sup>69</sup> This can lead to a false-negative result in  $\bullet\text{NO}$  detection.

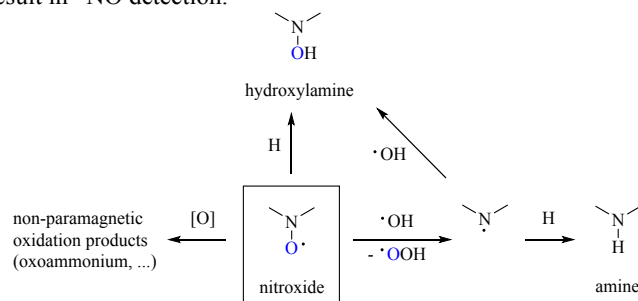


**Scheme 3. The loss of nitroxide moiety via reactions with plasma-induced ROS.**

Despite its limitations, ESR analysis is the most demonstrative tool in analyzing the mixture of (radical) RONS produced by cold plasma in liquids. Moreover, a useful technique of spin trapping can be used in combination with other techniques, as we show below.

### 3.3. Liquid chromatography and mass spectrometry of chemical substrates modified by RONS: Less direct, less selective.

The spin trapping technique discussed in previous section can be used in combination with (tandem) mass spectrometry. The adducts of DMPO, DEPMPO and other nitrene spin traps can be analysed not by EPR, but instead using liquid chromatography-mass spectrometry (LC-MS).<sup>97,98</sup> Certainly, this technique needs to be used with caution, as nitroxides may decay during the analysis, e.g. during electrospray ionisation.<sup>99</sup>

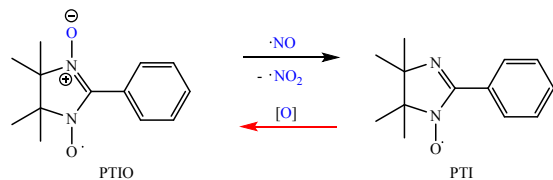

**Scheme 4. Formation of imino nitroxide PTI via reaction of nitronyl nitroxide PTIO with  $\bullet\text{NO}$ . A reverse reaction is marked with a red arrow.**

In general, mass spectrometry is a versatile technique that can be used for the analysis of stable products, formed in reactions of chemicals with plasma-induced RONS. However, just like with any other method, the complexity of plasma-liquid systems arises from the large variety of RONS in the gas phase plasma, which creates selectivity concerns.

Amino acids, such as e.g. cysteine, are viable ‘fingerprint’ probes for the detection of RONS in solutions exposed to CAP. Depending on the dominant RONS present in different plasmas, cysteine undergoes different transformations, which can be tracked using the MS analysis of the products.<sup>100,101</sup> The

presence of  $\text{ONOO}^-$  and  $\text{ClO}^-$  (a highly oxidising and bio-effective species formed upon plasma exposure of chloride-containing solutions<sup>44,91</sup>) in plasma-treated media can also be assessed using LC-MS. The detection is based on the mass spectrometric analysis of the modified L-tyrosine in aqueous media after plasma exposure. Here, one of the formed products, 3-nitrotyrosine, is ascribed to originate from  $\text{ONOO}^-$  and  $\bullet\text{NO}$  radicals formed by CAP.<sup>102,103</sup> However, the nitration of tyrosine is highly non-selective, and can occur in reactions not only with  $\text{ONOO}^-$  and  $\bullet\text{NO}$ , but also  $\bullet\text{NO}_2$ ,  $\text{NO}_2^-$ , etc.<sup>104</sup> This limits the applicability of the method to a general presence of RNS in CAP-liquid systems rather than specific species.

Aromatic substitution reactions of phenol enable detection of O as well as  $\bullet\text{NO}$ ,  $\bullet\text{NO}_2$ , and  $\bullet\text{OH}$  radicals. Nitration and nitrosation of phenols with subsequent high performance liquid chromatography (HPLC) analysis of the products can be used to detect  $\text{ONOO}^-$  in aqueous solutions after exposure to CAP. Although several species can lead to the formation of the same product (e.g., nitrosophenol is formed with both  $\bullet\text{NO}$  and  $\text{ONOO}^-$ ; nitrophenol with  $\bullet\text{NO}_2$ ,  $\text{HNO}_2$  and  $\text{HNO}_3$ ), the dominating reactions are highly pH dependent.<sup>36</sup> Similarly, HPLC analysis of the hydroxylated products of phenol can be used to detect  $\bullet\text{OH}$  in liquids in contact with plasma.<sup>42</sup> However, the selectivity is once again an issue: this hydroxylation can also occur with CAP-produced solvated O atoms.<sup>105,106</sup>

HPLC can be employed without MS analysis. This requires calibration of the HPLC equipment with the analysed compounds. Salicylic acid (SA) is used in CAP-water systems, for the detection of plasma-produced  $\bullet\text{OH}$ . HPLC (even without MS) can be used to detect the hydroxylation product of SA: 2,5-dihydroxybenzoic acid (2,5-DHBA).<sup>107</sup> It was also shown that reactions of SA with  $\bullet\text{OH}$  in CAP-treated aqueous media lead not only to 2,5-DHBA, but also 2,3-DHBA and catechol.<sup>108</sup> HPLC analysis thus requires initial calibration of the specific method (eluent, column, flow, etc.) to estimate the retention time of the products, and thus obtain quantitative results on their concentrations. However, it has not been taken into account that the hydroxylated product formation is likely non-selective: it can be caused by  $\text{O}_3$ <sup>109</sup> and possibly O atoms (similarly to reactions of phenols; see above).

Thus, the quantitative measurements require assessment of all reaction products, and are largely influenced by the presence of other plasma-induced RONS (Scheme 5).

Aqueous solutions of dimethylsulfoxide were employed in the detection of  $\bullet\text{OH}$  as well. The products of the reaction, formaldehyde (HCHO) and methanesulfinic acid, are analysed e.g. by HPLC (HCHO is first subjected to derivatisation with 2,4-dinitrophenyl hydrazine).<sup>57,110,111</sup> However, the results may not be quantitative due to the possible degradation of the analysed product: HCHO is over-oxidised to  $\text{CO}_2$  by  $\bullet\text{OH}$  in the presence of  $\text{O}_2$ .<sup>111</sup>

Thus, chromatography and/or mass spectrometry present valuable analytical options for the analysis of plasma-produced RONS in liquids, albeit not always quantitatively straightforward. Chemical modification of substrates may be non-selective and require complex optimisation of analytical conditions together with careful kinetic considerations.

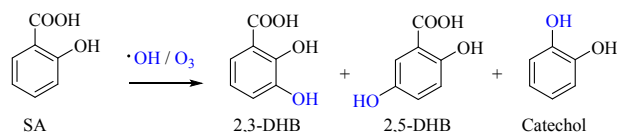
Scheme 5. Reaction of salicylic acid (SA) with  $\cdot\text{OH}$  and  $\text{O}_3$ .

Table 1. Analytical techniques used for the detection of short-lived RONS created in plasma-air-water systems.

Analytical technique	Plasma RONS detected	Advantages	Limitations
UV-Vis spectrophotometry, fluorimetry	$\cdot\text{OH}$ , $\text{O}_2\cdot^-$ , $\text{O}$ , $\text{O}_3$ , $\text{ONOO}^-$	Analysed compounds are stable. Presence of many RONS can be visualised. Non-destructive.	Indirect. Highly non-selective degradation of dyes. Non-selective induction of chemiluminescence or fluorescence.
HPLC, LC-MS(MS)	$\cdot\text{OH}$ , $\text{O}_2\cdot^-/\cdot\text{OOH}$ , $\text{O}$ , $\text{O}_3$ , $\cdot\text{NO}$ , $\cdot\text{NO}_2$ , $\text{ONOO}^-$	Analysed compounds are (often) stable.	Indirect. Non-selectivity of the reactions of chemical probes with plasma-induced RONS.
ESR spectroscopy	$\cdot\text{OH}$ , $\text{O}_2\cdot^-/\cdot\text{OOH}$ , $\text{O}$ , $\text{O}_3$ , $^1\text{O}_2$ , $\text{H}$ , $\cdot\text{NO}$ , $\text{ONOO}^-$	The most direct method. More selective than others. Many radicals can be identified simultaneously from the same spectrum. Non-destructive.	Non-selective formation of nitroxides from hydroxylamine spin probes. Non-selective formation of spin trap adducts. Oxidative degradation of spin traps by plasma RONS. Decay of spin adducts by plasma RONS: inherent, nitroxide reactions, oxidation of PTI back to PTIO.

#### 4. Summary and perspectives.

In this Feature Article, we discussed the possibilities of the main analytical methods used for the detection of short-lived RONS induced by CAP in liquids. Many of these methods are directly adapted from biological and chemical systems. In these environments, the analytical techniques are based on spin trapping or substrate ('probe') modification with subsequent LC, MS, ESR, or UV-Vis analyses.

The main difference between cold plasma-air-water systems and traditional biological and chemical systems is that in CAP, all (or many) types of RONS are present at the same time. This results in non-selective formation of products (e.g. hydroxylation of phenol), non-selective induction/decay of colour or fluorescence (methylene blue reactions with  $\cdot\text{OH}$  and  $\text{O}_3$ ), enhanced degradation of spin traps/spin adducts, etc. This is summarised in Table 1.

We also discuss the limitations of the methods in general, applicable in a wide range of systems with short-lived RONS. Some of the limitations of e.g. spin trapping are universal, and should be taken into account during analysis.

Besides the short-lived RONS discussed above, some other may be present in plasma-treated liquids, and their detection and quantification is required. For example, peroxyxynitrite ( $\text{ONOO}^-$ ) is a 'sought-after' chemical compound in CAP-water systems,<sup>112</sup> but peroxyxynitrate ( $\text{OONOO}^-$ ) is rarely mentioned, although it can be responsible for most of the bactericidal action of plasma in liquids.<sup>113</sup> Solvated electrons delivered by CAP can initiate radical reactions,<sup>18,114</sup> but their detection in liquids so far has been limited to spectroscopy with a laser diode array<sup>115</sup> and pH measurements in a chlor-alkali process.<sup>116</sup> Like peroxyxynitric acid<sup>117</sup> or other RONS, free electrons are induced in the media only by some types of CAP: this depends on the configuration of the CAP system.<sup>5,32,33,35</sup>

This means that *not all plasmas are created equal*: the 'cocktail' of reactive species produced in a dielectric barrier discharge (DBD) can be different from that created by an Ar plasma jet. For example,  $^1\text{O}_2$  is created only by some plasma jets,<sup>72</sup> but not by others.<sup>33</sup> This is not to mention various

configurations of the jets or DBDs.<sup>35</sup> Accordingly, the analytical methods should be selected as best suited not only for specific reactive species, but also for the specific CAP-air-water system. The limitations of the analysis methods are general, but in some cases RONS that can interfere with the analytical procedures are simply not present.

Careful choice of analytical methods, optimisation of analytical procedures, and comprehensive control experiments can provide an expanded view of the plasma-air-water systems. The complete understanding of such systems, using the expertise from chemistry, biology, and physics, is required for their further development and tailored applications in chemistry, agriculture, food industry, and medicine.

#### AUTHOR INFORMATION

Yury Gorbanev is a Marie Curie postdoctoral research fellow at PLASMANT, University of Antwerp, working on analysis and development of biomedical cold plasma. He previously participated in an interdisciplinary research project between the Department of Chemistry and York Plasma Institute, University of York, UK, dealing with chemical characteristics and various applications of cold atmospheric plasmas. Angela Privat-Maldonado is a postdoctoral researcher at PLASMANT. She investigates the biological effects and anti-tumour capabilities of cold plasmas. Annemie Bogaerts is Head of the PLASMANT research group, with research interests in fundamental properties, as well as industrial and biomedical applications, of cold plasma. She leads many collaborative projects, including both computational and experimental research on chemical processes in cold plasmas.

#### Corresponding Author

\* Phone: +32(0)32652343, email: yury.gorbanev@uantwerpen.be.

#### Author Contributions

The manuscript was written through contributions of all authors. All authors have given approval to the final version of the manuscript.



## ACKNOWLEDGMENT

This work was supported by the European Marie Skłodowska-Curie Individual Fellowship within Horizon2020 ('LTPAM', grant no. 743151).

## REFERENCES

- (1) Burm, K. T. A. L. Plasma: The Fourth State of Matter. *Plasma Chem. Plasma Process.* **2012**, *32*, 401-407.
- (2) Bogaerts, A.; Neyts, E.; Gijbels, R.; van der Mullen, J. Gas discharge plasmas and their applications. *Spectrochim. Acta B: At. Spectrosc.* **2002**, *57*, 609-658.
- (3) Nehra, V.; Kumar, A.; Dwivedi, H. K. Atmospheric Non-Thermal Plasma Sources. *Int. J. Eng.* **2008**, 53-68.
- (4) Smoluch, M.; Mielczarek, P.; Silberring, J. Plasma-based ambient ionization mass spectrometry in bioanalytical sciences. *Mass Spectrom. Rev.* **2015**, *35*, 22-34.
- (5) Adamovich, I.; Baalrud, S. D.; Bogaerts, A.; Bruggeman, P. J.; Cappelli, M.; Colombo, V.; Czarnetzki, U.; Ebert, U.; Eden, J. G.; Favia, P., et al. The 2017 Plasma Roadmap: Low temperature plasma science and technology. *J. Phys. D: Appl. Phys.* **2017**, *50*, 323001.
- (6) Bogaerts, A.; Neyts, E. C. Plasma Technology: An Emerging Technology for Energy Storage. *ACS Energy Lett.* **2018**, *3*, 1013-1027.
- (7) Lu, X.; Naidis, G. V.; Laroussi, M.; Reuter, S.; Graves, D. B.; Ostrikov, K. Reactive species in non-equilibrium atmospheric-pressure plasmas: Generation, transport, and biological effects. *Phys. Rep.* **2016**, *630*, 1-84.
- (8) West, A.; Schans, M. v. d.; Xu, C.; Cooke, M.; Wagenaars, E. Fast, downstream removal of photoresist using reactive oxygen species from the effluent of an atmospheric pressure plasma jet. *Plasma Sources Sci. Technol.* **2016**, *25*, 02LT01.
- (9) Neyts, E. C.; Ostrikov, K.; Sunkara, M. K.; Bogaerts, A. Plasma Catalysis: Synergistic Effects at the Nanoscale. *Chem. Rev.* **2015**, *115*, 13408-13446.
- (10) Feng, X.; Liu, H.; He, C.; Shen, Z.; Wang, T. Synergistic effects and mechanism of a non-thermal plasma catalysis system in volatile organic compound removal: a review. *Catal. Sci. Technol.* **2018**, *8*, 936-954.
- (11) Zendeenam, A.; Ghasemi, J.; Zendeenam, A. Employing cold atmospheric plasma (Ar, He) on Ag thin film and their influences on surface morphology and anti-bacterial activity of silver films for water treatment. *Int. Nano Lett.* **2018**, *8*, 157-164.
- (12) Rezaei, F.; Gorbanev, Y.; Chys, M.; Nikiforov, A.; Van Hulle, S. W. H.; Cos, P.; Bogaerts, A.; De Geyter, N. Investigation of plasma-induced chemistry in organic solutions for enhanced electrospun PLA nanofibers. *Plasma Proc. Polym.* **2018**, *15*, 1700226.
- (13) Ramkumar, M. C.; Navaneetha Pandiyaraj, K.; Arun Kumar, A.; Padmanabhan, P. V. A.; Cools, P.; De Geyter, N.; Morent, R.; Uday Kumar, S.; Kumar, V.; Gopinath, P., et al. Atmospheric pressure non-thermal plasma assisted polymerization of poly (ethylene glycol) methylether methacrylate (PEGMA) on low density polyethylene (LDPE) films for enhancement of biocompatibility. *Surf. Coat. Technol.* **2017**, *329*, 55-67.
- (14) Vanraes, P.; Wardenier, N.; Surmont, P.; Lynen, F.; Nikiforov, A.; Van Hulle, S. W. H.; Leys, C.; Bogaerts, A. Removal of alachlor, diuron and isoproturon in water in a falling film dielectric barrier discharge (DBD) reactor combined with adsorption on activated carbon textile: Reaction mechanisms and oxidation by-products. *J. Hazard. Mater.* **2018**, *354*, 180-190.
- (15) Mustafa, M. F.; Fu, X.; Liu, Y.; Abbas, Y.; Wang, H.; Lu, W. Volatile organic compounds (VOCs) removal in non-thermal plasma double dielectric barrier discharge reactor. *J. Hazard. Mater.* **2018**, *347*, 317-324.
- (16) Snoeckx, R.; Bogaerts, A. Plasma technology – a novel solution for CO<sub>2</sub> conversion? *Chem. Soc. Rev.* **2017**, *46*, 5805-5863.
- (17) Zhang, M.; Ognier, S.; Touati, N.; Hauner, I.; Guyon, C.; Binet, L.; Tatoulian, M. A plasma/liquid microreactor for radical reaction chemistry: An experimental and numerical investigation by EPR spin trapping. *Plasma Proc. Polym.* **2017**, *15*, 1700188.
- (18) Gorbanev, Y.; Leifert, D.; Studer, A.; O'Connell, D.; Chechik, V. Initiating radical reactions with non-thermal plasmas. *Chem. Commun.* **2017**, *53*, 3685-3688.
- (19) Puač, N.; Gherardi, M.; Shiratani, M. Plasma agriculture: A rapidly emerging field. *Plasma Proc. Polym.* **2017**, *15*, 1700174.
- (20) Thirumdas, R.; Sarangapani, C.; Annapure, U. S. Cold Plasma: A novel Non-Thermal Technology for Food Processing. *Food Biophys.* **2015**, *10*, 1-11.
- (21) Arora, V.; Nikhil, V.; Suri, N. K.; Arora, P. Cold Atmospheric Plasma (CAP) in Dentistry. *Dentistry* **2014**, *4*, 189.
- (22) Ranjan, R.; Krishnamraju, P. V.; Shankar, T.; Gowd, S. J. *Int. Soc. Prevent. Communit. Dent.* **2017**, *7*, 71-75.
- (23) Nikiforov, A.; Xiaolong, D.; Qing, X.; Cvelbar, U.; DeGeyter, N.; Morent, R.; Christophe, L. Non-thermal plasma technology for the development of antimicrobial surfaces: a review. *J. Phys. D: Appl. Phys.* **2016**, *49*, 204002.
- (24) Weltmann, K. D.; von Woedtke, T. Plasma medicine—current state of research and medical application. *Plasma Phys. Control. Fusion* **2017**, *59*, 014031.
- (25) Laroussi, M. Plasma Medicine: A Brief Introduction. *Plasma* **2018**, *1*, 47-60.
- (26) Aoubakr, H. A.; Gangal, U.; Youssef, M. M.; Goyal, S. M.; Bruggeman, P. J. Inactivation of virus in solution by cold atmospheric pressure plasma: identification of chemical inactivation pathways. *J. Phys. D: Appl. Phys.* **2016**, *49*, 204001.
- (27) Privat-Maldonado, A.; Gorbanev, Y.; O'Connell, D.; Vann, R.; Chechik, V.; van der Woude, M. W. Nontarget Biomolecules Alter Macromolecular Changes Induced by Bactericidal Low-Temperature Plasma. *IEEE Trans. Radiat. Plasma Med. Sci.* **2018**, *2*, 121-128.
- (28) Vermeylen, S.; De Waele, J.; Vanuytsel, S.; De Backer, J.; Van der Paal, J.; Ramakers, M.; Leyssens, K.; Marcq, E.; Van Audenaerde, J.; Smits, E. L. J., et al. Cold atmospheric plasma treatment of melanoma and glioblastoma cancer cells. *Plasma Proc. Polym.* **2016**, *13*, 1195-1205.
- (29) Reiazi, R.; Akbari, M. E.; Norozi, A.; Etedadialibadi, M. Application of Cold Atmospheric Plasma (CAP) in Cancer Therapy: A Review. *Int. J. Cancer Manag.* **2017**, *10*, e8728.
- (30) Van Boxem, W.; Van der Paal, J.; Gorbanev, Y.; Vanuytsel, S.; Smits, E.; Dewilde, S.; Bogaerts, A. Anti-cancer capacity of plasma-treated PBS: effect of chemical composition on cancer cell cytotoxicity. *Sci. Rep.* **2017**, *7*, 16478.
- (31) Attri, P.; Kumar, N.; Park, J. H.; Yadav, D. K.; Choi, S.; Uhm, H. S.; Kim, I. T.; Choi, E. H.; Lee, W. Influence of reactive species on the modification of biomolecules generated from the soft plasma. *Sci. Rep.* **2015**, *5*, 8221.
- (32) Gorbanev, Y.; Verlactt, C. C. W.; Tinck, S.; Tuenter, E.; Foubert, K.; Cos, P.; Bogaerts, A. Combining experimental and modelling approaches to study the sources of reactive species induced in water by the COST RF plasma jet. *Phys. Chem. Chem. Phys.* **2018**, *20*, 2797-2808.
- (33) Gorbanev, Y.; O'Connell, D.; Chechik, V. Non-Thermal Plasma in Contact with Water: The Origin of Species. *Chem. Eur. J.* **2016**, *22*, 3496-3505.
- (34) Norberg, S. A.; Tian, W.; Johnsen, E.; Kushner, M. J. Atmospheric pressure plasma jets interacting with liquid covered tissue: touching and not-touching the liquid. *J. Phys. D: Appl. Phys.* **2014**, *47*, 475203.
- (35) Bruggeman, P. J.; Kushner, M. J.; Locke, B. R.; Gardeniers, J. G. E.; Graham, W. G.; Graves, D. B.; Hofman-Caris, R. C. H. M.; Maric, D.; Reid, J. P.; Ceriani, E., et al. Plasma-liquid interactions: a review and roadmap. *Plasma Sources Sci. Technol.* **2016**, *25*, 053002.
- (36) Lukes, P.; Dolezalova, E.; Sisrova, I.; Clupek, M. Aqueous-phase chemistry and bactericidal effects from an air discharge plasma in contact with water: evidence for the formation of peroxyxynitrite through a pseudo-second-order post-discharge reaction of H<sub>2</sub>O<sub>2</sub> and HNO<sub>2</sub>. *Plasma Sources Sci. Technol.* **2014**, *23*, 015019.

- (37) Babaeva, N. Y.; Naidis, G. V. Modeling of Plasmas for Biomedicine. *Trends Biotechnol.* **2018**, *36*, 603-614.
- (38) Verlackt, C. C. W.; Neyts, E. C.; Bogaerts, A. Atomic scale behavior of oxygen-based radicals in water. *J. Phys. D: Appl. Phys.* **2017**, *50*, 11LT01.
- (39) Verlackt, C. C. W.; Van Boxem, W.; Bogaerts, A. Transport and accumulation of plasma generated species in aqueous solution. *Phys. Chem. Chem. Phys.* **2018**, *20*, 6845-6859.
- (40) Yan, D.; Nourmohammadi, N.; Bian, K.; Murad, F.; Sherman, J. H.; Keidar, M. Stabilizing the cold plasma-stimulated medium by regulating medium's composition. *Sci. Rep.* **2016**, *6*, 26016.
- (41) Massima Mouele, E. S.; Fatoba, O. O.; Babajide, O. Review of the methods for determination of reactive oxygen species and suggestion for their application in advanced oxidation induced by dielectric barrier discharges. *Environ. Sci. Pollut. Res. Int.* **2018**, *25*, 9265-9282.
- (42) Tarabová, B.; Lukeš, P.; Janda, M.; Hensel, K.; Šikurová, L.; Machala, Z. Specificity of detection methods of nitrites and ozone in aqueous solutions activated by air plasma. *Plasma Proc. Polym.* **2018**, *15*, 1800030.
- (43) Sasaki, S.; Kanzaki, M.; Kaneko, T. Calcium influx through TRP channels induced by short-lived reactive species in plasma-irradiated solution. *Sci. Rep.* **2016**, *6*, 25728.
- (44) Kondeti, V. S. S. K.; Phan, C. Q.; Wende, K.; Jablonowski, H.; Gangal, U.; Granick, J. L.; Hunter, R. C.; Bruggeman, P. J. Long-lived and short-lived reactive species produced by a cold atmospheric pressure plasma jet for the inactivation of *Pseudomonas aeruginosa* and *Staphylococcus aureus*. *Free Radic. Biol. Med.* **2018**, *124*, 275-287.
- (45) Bekeschus, S.; Wende, K.; Hefny, M. M.; Rödder, K.; Jablonowski, H.; Schmidt, A.; Woedtke, T. v.; Weltmann, K.-D.; Benedikt, J. Oxygen atoms are critical in rendering THP-1 leukaemia cells susceptible to cold physical plasma-induced apoptosis. *Sci. Rep.* **2017**, *7*, 2791.
- (46) Lin, A.; Gorbanev, Y.; Cos, P.; Smits, E.; Bogaerts, A. Plasma Elicits Immunogenic Death In Melanoma Cells. *Clin. Plasma Med.* **2018**, *9*, 9.
- (47) Attri, P.; Yusupov, M.; Park, J. H.; Lingamdinne, L. P.; Koduru, J. R.; Shiratani, M.; Choi, E. H.; Bogaerts, A. Mechanism and comparison of needle-type non-thermal direct and indirect atmospheric pressure plasma jets on the degradation of dyes. *Sci. Rep.* **2016**, *6*, 34419.
- (48) Yuichiro, T.; Naohiro, Y.; Tamio, H. Decomposition of Methylene Blue by using an Atmospheric Plasma Jet with Ar, N<sub>2</sub>, O<sub>2</sub>, or Air. *Jap. J. Appl. Phys.* **2013**, *52*, 056102.
- (49) Girard, F.; Badets, V.; Blanc, S.; Gazeli, K.; Marlin, L.; Authier, L.; Svarnas, P.; Sojic, N.; Clément, F.; Arbault, S. Formation of reactive nitrogen species including peroxyxynitrite in physiological buffer exposed to cold atmospheric plasma. *RSC Adv.* **2016**, *6*, 78457-78467.
- (50) Bekeschus, S.; Schmidt, A.; Niessner, F.; Gerling, T.; Weltmann, K.-D.; Wende, K. Basic Research in Plasma Medicine - A Throughput Approach from Liquids to Cells. *J. Vis. Exp.* **2017**, e56331.
- (51) García, M. C.; Mora, M.; Esquivel, D.; Foster, J. E.; Rodero, A.; Jiménez-Sanchidrián, C.; Romero-Salguero, F. J. Microwave atmospheric pressure plasma jets for wastewater treatment: Degradation of methylene blue as a model dye. *Chemosphere* **2017**, *180*, 239-246.
- (52) Zhao, Y. Y.; Wang, T.; MacGregor, S. J.; Wilson, M. P.; Given, M. J.; Timoshkin, I. V. In *Proceedings of the 20th International Conference on Gas Discharges and their Applications*, 2014, pp 566-569.
- (53) Hayyan, M.; Hashim, M. A.; AlNashef, I. M. Superoxide Ion: Generation and Chemical Implications. *Chem. Rev.* **2016**, *116*, 3029-3085.
- (54) Naoki, S.; Yutaka, M.; Koichi, S. Visualization of short-lived reactive species in liquid in contact with atmospheric-pressure plasma by chemiluminescence of luminol. *Appl. Phys. Express* **2018**, *11*, 026201.
- (55) Kim, S. J.; Chung, T. H. Cold atmospheric plasma jet-generated RONS and their selective effects on normal and carcinoma cells. *Sci. Rep.* **2016**, *6*, 20332.
- (56) Uchiyama, H.; Zhao, Q.-L.; Hassan, M. A.; Andocs, G.; Nojima, N.; Takeda, K.; Ishikawa, K.; Hori, M.; Kondo, T. EPR-Spin Trapping and Flow Cytometric Studies of Free Radicals Generated Using Cold Atmospheric Argon Plasma and X-Ray Irradiation in Aqueous Solutions and Intracellular Milieu. *PLoS One* **2015**, *10*, e0136956.
- (57) Sahni, M.; Locke, B. R. Quantification of Hydroxyl Radicals Produced in Aqueous Phase Pulsed Electrical Discharge Reactors. *Ind. Eng. Chem. Res.* **2006**, *45*, 5819-5825.
- (58) Attri, P.; Kim, Y. H.; Park, D. H.; Park, J. H.; Hong, Y. J.; Uhm, H. S.; Kim, K.-N.; Fridman, A.; Choi, E. H. Generation mechanism of hydroxyl radical species and its lifetime prediction during the plasma-initiated ultraviolet (UV) photolysis. *Sci. Rep.* **2015**, *5*, 9332.
- (59) Chandrasekara Pillai, K.; Kwon, T. O.; Moon, I. S. Degradation of wastewater from terephthalic acid manufacturing process by ozonation catalyzed with Fe<sup>2+</sup>, H<sub>2</sub>O<sub>2</sub> and UV light: Direct versus indirect ozonation reactions. *Appl. Cat. B: Environ.* **2009**, *91*, 319-328.
- (60) Szili, E. J.; Bradley, J. W.; Short, R. D. A 'tissue model' to study the plasma delivery of reactive oxygen species. *J. Phys. D: Appl. Phys.* **2014**, *47*, 152002.
- (61) Chechik, V.; Carter, E.; Murphy, D. *Electron Paramagnetic Resonance*; Oxford University Press: Oxford, UK, 2016.
- (62) Kohno, M. Applications of Electron Spin Resonance Spectrometry for Reactive Oxygen Species and Reactive Nitrogen Species Research. *J. Clin. Biochem. Nutr.* **2010**, *47*, 1-11.
- (63) Stolze, K.; Rohr-Udilova, N.; Rosenau, T.; Stadtmüller, R.; Nohl, H. Very stable superoxide radical adducts of 5-ethoxycarbonyl-3,5-dimethyl-pyrroline N-oxide (3,5-EDPO) and its derivatives. *Biochem. Pharmacol.* **2005**, *69*, 1351-1361.
- (64) Bagryanskaya, E. G.; Krumkacheva, O. A.; Fedin, M. V.; Marke, S. R. A. In *Methods Enzymol.*, Qin, P. Z.; Warncke, K., Eds.; Academic Press, 2015, pp 365-396.
- (65) Suzen, S.; Gurer-Orhan, H.; Saso, L. Detection of Reactive Oxygen and Nitrogen Species by Electron Paramagnetic Resonance (EPR) Technique. *Molecules* **2017**, *22*, 181.
- (66) Wu, H.; Sun, P.; Feng, H.; Zhou, H.; Wang, R.; Liang, Y.; Lu, J.; Zhu, W.; Zhang, J.; Fang, J. Reactive Oxygen Species in a Non-thermal Plasma Microjet and Water System: Generation, Conversion, and Contributions to Bacteria Inactivation—An Analysis by Electron Spin Resonance Spectroscopy. *Plasma Proc. Polym.* **2012**, *9*, 417-424.
- (67) Tresp, H.; Hammer, M. U.; Winter, J.; Weltmann, K. D.; Reuter, S. Quantitative detection of plasma-generated radicals in liquids by electron paramagnetic resonance spectroscopy. *J. Phys. D: Appl. Phys.* **2013**, *46*, 435401.
- (68) Tani, A.; Ono, Y.; Fukui, S.; Ikawa, S.; Kitano, K. Free radicals induced in aqueous solution by non-contact atmospheric-pressure cold plasma. *Appl. Phys. Lett.* **2012**, *100*, 254103.
- (69) Gorbanev, Y.; Stehling, N.; O'Connell, D.; Chechik, V. Reactions of nitroxide radicals in aqueous solutions exposed to non-thermal plasma: limitations of spin trapping of the plasma induced species. *Plasma Sources Sci. Technol.* **2016**, *25*, 055017.
- (70) Chauvin, J.; Judée, F.; Yousfi, M.; Vicendo, P.; Merbahi, N. Analysis of reactive oxygen and nitrogen species generated in three liquid media by low temperature helium plasma jet. *Sci. Rep.* **2017**, *7*, 4562.
- (71) Elg, D. T.; Yang, I. W.; Graves, D. B. Production of TEMPO by O atoms in atmospheric pressure non-thermal plasma-liquid interactions. *J. Phys. D: Appl. Phys.* **2017**, *50*, 475201.
- (72) Takamatsu, T.; Uehara, K.; Sasaki, Y.; Miyahara, H.; Matsumura, Y.; Iwasawa, A.; Ito, N.; Azuma, T.; Kohno, M.; Okino, A. Investigation of reactive species using various gas plasmas. *RSC Adv.* **2014**, *4*, 39901-39905.
- (73) Gorbanev, Y.; Soriano, R.; O'Connell, D.; Chechik, V. An Atmospheric Pressure Plasma Setup to Investigate the Reactive Species Formation. *J. Vis. Exp.* **2016**, e54765.

- (74) Uchiyama, H.; Ishikawa, K.; Zhao, Q. L.; Andocs, G.; Nojima, N.; Takeda, K.; Krishna, M. C.; Ishijima, T.; Matsuya, Y.; Hori, M., et al. Free radical generation by non-equilibrium atmospheric pressure plasma in alcohol–water mixtures: an EPR-spin trapping study. *J. Phys. D: Appl. Phys.* **2018**, *51*, 095202.
- (75) Guo, L.; Xu, R.; Gou, L.; Liu, Z.; Zhao, Y.; Liu, D.; Zhang, L.; Chen, H.; Kong, M. G. *Appl. Environ. Microbiol.* **2018**, DOI: 10.1128/AEM.00726-18.
- (76) Xu, H.; Chen, C.; Liu, D.; Xu, D.; Liu, Z.; Wang, X.; Kong, M. G. Contrasting characteristics of aqueous reactive species induced by cross-field and linear-field plasma jets. *J. Phys. D: Appl. Phys.* **2017**, *50*, 245201.
- (77) Wetherill, L. F. Can ESR be used to assess the levels of oxidative stress in fat-loaded human hepatocytes and hepatic stellate cells? *Biosci. Horiz.* **2009**, *2*, 197-204.
- (78) Torfs, E.; Vajs, J.; Macedo Maira, B.; Cools, F.; Vanhoutte, B.; Gorbanev, Y.; Bogaerts, A.; Verschaeve, L.; Caljon, G.; Maes, L., et al. Synthesis and in vitro investigation of halogenated 1,3-bis(4-nitrophenyl)triazene salts as antitubercular compounds. *Chem. Biol. Drug Des.* **2017**, *91*, 631-640.
- (79) Radi, R. Peroxynitrite, a stealthy biological oxidant. *J. Biol. Chem.* **2013**, *288*, 26464-26472.
- (80) Tsuchiya, K.; Yoshizumi, M.; Houchi, H.; Mason, R. P. Nitric oxide-forming reaction between the iron-N-methyl-D-glucamine dithiocarbamate complex and nitrite. *J. Biol. Chem.* **2000**, *275*, 1551-1556.
- (81) Forrester, A. R.; Hepburn, S. P. Spin traps. A cautionary note. *J. Chem. Soc. C: Org.* **1971**, 701-703.
- (82) Rhodes, C. J. *Toxicology of the Human Environment: The Critical Role of Free Radicals.*; CRC Press: Boca Raton, Florida, USA, 2000.
- (83) Šeršeň, F.; Kráľová, K. In *Photosynthesis*, Dubinsky, Z., Ed.; IntechOpen, 2013, pp 247-283.
- (84) Betterton, E. A.; Craig, D. Kinetics and Mechanism of the Reaction of Azide with Ozone in Aqueous Solution. *J. Air Waste Manag. Assoc.* **1999**, *49*, 1347-1354.
- (85) Buettner, G. R.; Oberley, L. W. Considerations in the spin trapping of superoxide and hydroxyl radical in aqueous systems using 5,5-dimethyl-1-pyrroline-1-oxide. *Biochem. Biophys. Res. Commun.* **1978**, *83*, 69-74.
- (86) Buettner, G. R. *Free Radic. Res. Commun.* **1993**, *19*, S79-S87.
- (87) Thagard, S. M.; Stratton, G. R.; Dai, F.; Bellona, C. L.; Holsen, T. M.; Bohl, D. G.; Paek, E.; Dickenson, E. R. V. Plasma-based water treatment: development of a general mechanistic model to estimate the treatability of different types of contaminants. *J. Phys. D: Appl. Phys.* **2017**, *50*, 014003.
- (88) Magureanu, M.; Bradu, C.; Parvulescu, V. I. Plasma processes for the treatment of water contaminated with harmful organic compounds. *J. Phys. D: Appl. Phys.* **2018**, *51*, 313002.
- (89) Moreno, S. N. J.; Stolze, K.; Janzen, E. G.; Mason, R. P. Oxidation of cyanide to the cyanyl radical by peroxidase/H<sub>2</sub>O<sub>2</sub> systems as determined by spin trapping. *Archiv. Biochem. Biophys.* **1988**, *265*, 267-271.
- (90) Mareike, A. C. H.; Miriam, M.; Klaus-Dieter, W.; Thomas von, W. Analysis of antibacterial efficacy of plasma-treated sodium chloride solutions. *J. Phys. D: Appl. Phys.* **2015**, *48*, 454001.
- (91) Hänsch, M. A. C.; Mann, M.; Weltmann, K. D.; von Woedtke, T. Analysis of antibacterial efficacy of plasma-treated sodium chloride solutions. *J. Phys. D: Appl. Phys.* **2015**, *48*, 454001.
- (92) Bernofsky, C.; Bandara, B. M. R.; Hinojosa, O. Electron spin resonance studies of the reaction of hypochlorite with 5,5-dimethyl-1-pyrroline-N-oxide. *Free Radic. Biol. Med.* **1990**, *8*, 231-239.
- (93) Brandenburg, R. Dielectric barrier discharges: progress on plasma sources and on the understanding of regimes and single filaments. *Plasma Sources Sci. Technol.* **2017**, *26*, 053001.
- (94) Marshall, D. L.; Christian, M. L.; Gryn'ova, G.; Coote, M. L.; Barker, P. J.; Blanksby, S. J. Oxidation of 4-substituted TEMPO derivatives reveals modifications at the 1- and 4-positions. *Org. Biomol. Chem.* **2011**, *9*, 4936-4947.
- (95) Goldstein, S.; Samuni, A.; Merenyi, G. Reactions of Nitric Oxide, Peroxynitrite, and Carbonate Radicals with Nitroxides and Their Corresponding Oxoammonium Cations. *Chem. Res. Toxicol.* **2004**, *17*, 250-257.
- (96) Hogg, N. Detection of nitric oxide by electron paramagnetic resonance spectroscopy. *Free Radic. Biol. Med.* **2010**, *49*, 122-129.
- (97) Guo, Q.; Qian, S. Y.; Mason, R. P. Separation and identification of DMPO adducts of oxygen-centered radicals formed from organic hydroperoxides by HPLC-ESR, ESI-MS and MS/MS. *J. Am. Soc. Mass Spectrom.* **2003**, *14*, 862-871.
- (98) Tuccio, B.; Lauricella, R.; Charles, L. Characterisation of free radical spin adducts of the cyclic β-phosphorylated nitron DEPMPPO using tandem mass spectrometry. *International Journal of Mass Spectrometry* **2006**, *252*, 47-53.
- (99) Zoia, L.; Argyropoulos, D. S. Characterization of Free Radical Spin Adducts of 5-Diisopropoxy-Phosphoryl-5-Methyl-1-Pyrroline-N-Oxide Using Mass Spectrometry and 31P Nuclear Magnetic Resonance. *Eur. J. Mass Spectrom.* **2010**, *16*, 175-185.
- (100) Bruno, G.; Heusler, T.; Jablonowski, H.; Lackmann, J.-W.; Wende, K. Mass Spectrometry Based Analysis Of The Oxidation Compounds Produced By Cold Atmospheric Plasma (CAP) Interaction With Cysteine. *Clin. Plasma Med.* **2018**, *9*, 33-34.
- (101) Lackmann, J. W.; Wende, K.; Verlact, C.; Golda, J.; Volzke, J.; Kogelheide, F.; Held, J.; Bekeschus, S.; Bogaerts, A.; Schulz-von der Gathen, V., et al. Chemical fingerprints of cold physical plasmas – an experimental and computational study using cysteine as tracer compound. *Sci. Rep.* **2018**, *8*, 7736.
- (102) Bekeschus, S.; Kolata, J.; Winterbourn, C.; Kramer, A.; Turner, R.; Weltmann, K. D.; Bröker, B.; Masur, K. Hydrogen peroxide: A central player in physical plasma-induced oxidative stress in human blood cells. *Free Radical Research* **2014**, *48*, 542-549.
- (103) Wende, K.; Williams, P.; Dalluge, J.; Van Gaens, W.; Aboubakr, H.; Bischof, J.; von Woedtke, T.; Goyal, S. M.; Weltmann, K.-D.; Bogaerts, A., et al. Identification of the biologically active liquid chemistry induced by a nonthermal atmospheric pressure plasma jet. *Biointerphases* **2015**, *10*, 029518.
- (104) Ahsan, H. 3-Nitrotyrosine: A biomarker of nitrogen free radical species modified proteins in systemic autoimmunogenic conditions. *Human Immunol.* **2013**, *74*, 1392-1399.
- (105) Hefny, M. M.; Pattyn, C.; Lukes, P.; Benedikt, J. Atmospheric plasma generates oxygen atoms as oxidizing species in aqueous solutions. *J. Phys. D: Appl. Phys.* **2016**, *49*, 404002.
- (106) Benedikt, J.; Mokhtar Hefny, M.; Shaw, A.; Buckley, B. R.; Iza, F.; Schäkermann, S.; Bandow, J. E. The fate of plasma-generated oxygen atoms in aqueous solutions: non-equilibrium atmospheric pressure plasmas as an efficient source of atomic O(aq). *Phys. Chem. Chem. Phys.* **2018**, *20*, 12037-12042.
- (107) Guo, Y.; Liao, X.; Ye, D. Detection of hydroxyl radical in plasma reaction on toluene removal. *J. Environ. Sci.* **2008**, *20*, 1429-1432.
- (108) Zhang, X.; Zhou, R.; Bazaka, K.; Liu, Y.; Zhou, R.; Chen, G.; Chen, Z.; Liu, Q.; Yang, S.; Ostrikov, K. Quantification of plasma produced OH radical density for water sterilization. *Plasma Proc. Polym.* **2018**, *15*, 1700241.
- (109) Hu, R.; Zhang, L.; Hu, J. Study on the kinetics and transformation products of salicylic acid in water via ozonation. *Chemosphere* **2016**, *153*, 394-404.
- (110) Kovačević, V. V.; P., D. B.; Jović, M.; M., R. G.; Obradović, B. M.; Kuraica, M. M. Measurement of reactive species generated by dielectric barrier discharge in direct contact with water in different atmospheres. *J. Phys. D: Appl. Phys.* **2017**, *50*, 155205.
- (111) Ma, Y.; X., G.; He, B.; X., L.; Cao, D.; J., L.; Xiong, Q.; Chen, Q.; Chen, B. H.; Liu, Q. H. On the quantification of the dissolved hydroxyl radicals in the plasma-liquid system using the molecular probe method. *J. Phys. D: Appl. Phys.* **2018**, *51*, 155205.

(112) Graves, D. B. Oxy-nitroso shielding burst model of cold atmospheric plasma therapeutics. *Clin. Plasma Med.* **2014**, *2*, 38-49.

(113) Satoshi, I.; Atsushi, T.; Yoichi, N.; Katsuhisa, K. Physicochemical properties of bactericidal plasma-treated water. *J. Phys. D: Appl. Phys.* **2016**, *49*, 425401.


(114) Lübbesmeyer, M.; Leifert, D.; Schäfer, H.; Studer, A. Electrochemical initiation of electron-catalyzed phenanthridine synthesis by trifluoromethylation of isonitriles. *Chem. Commun.* **2018**, *54*, 2240-2243.

(115) Rumbach, P.; Bartels, D. M.; Sankaran, R. M.; Go, D. B. The effect of air on solvated electron chemistry at a plasma/liquid interface. *J. Phys. D: Appl. Phys.* **2015**, *48*, 424001.


(116) Rumbach, P.; Bartels, D. M.; Sankaran, R. M.; Go, D. B. The solvation of electrons by an atmospheric-pressure plasma. *Nat. Commun.* **2015**, *6*, 7248.

(117) Kojtari, A.; Ercan, U. K.; Smith, J.; Friedman, G.; Sensenig, R. B.; Tyagi, S.; Joshi, S. G.; Ji, H. F.; Brooks, A. D. Chemistry for Antimicrobial Properties of Water Treated with Non-Equilibrium Plasma. *J. Nanomed. Biotherapeutic Discov.* **2013**, *4*, 1-5.

## TOC:

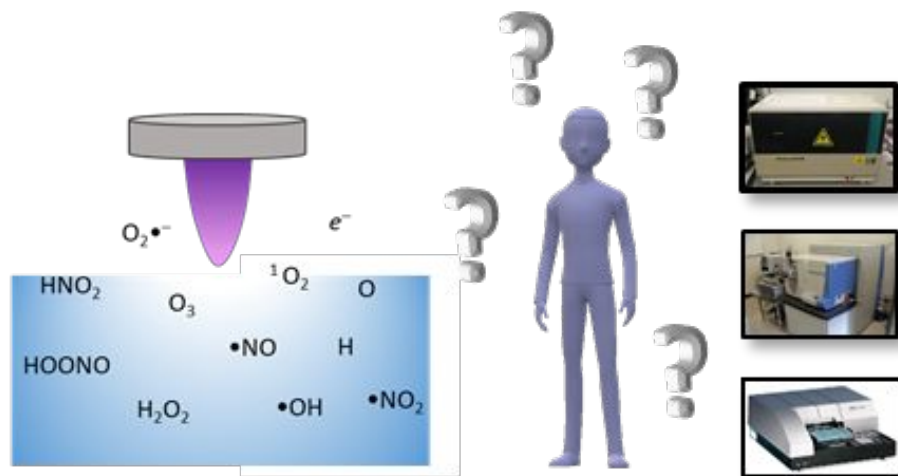




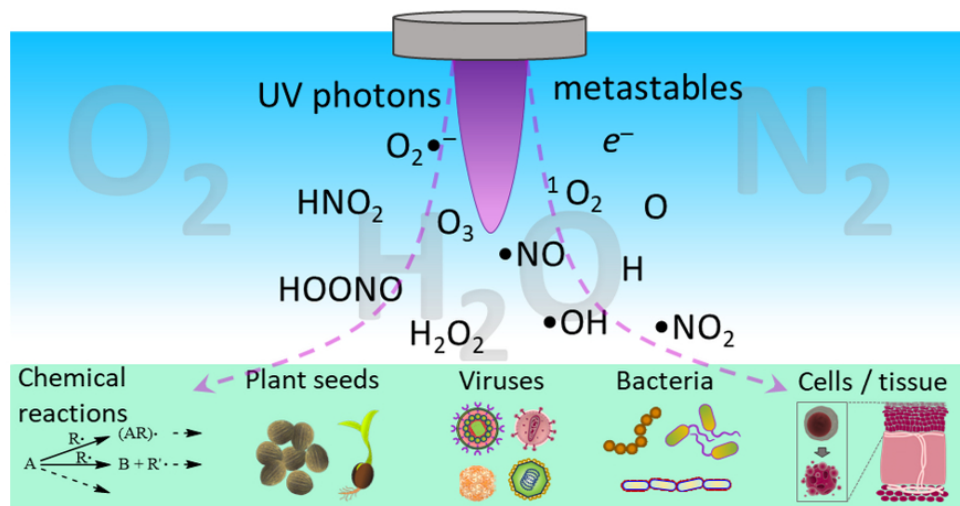

23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

Figure 1. Cold atmospheric pressure plasma in contact with liquids produces various reactive oxygen and nitrogen species for diverse chemical, agricultural and medical applications.

153x79mm (150 x 150 DPI)

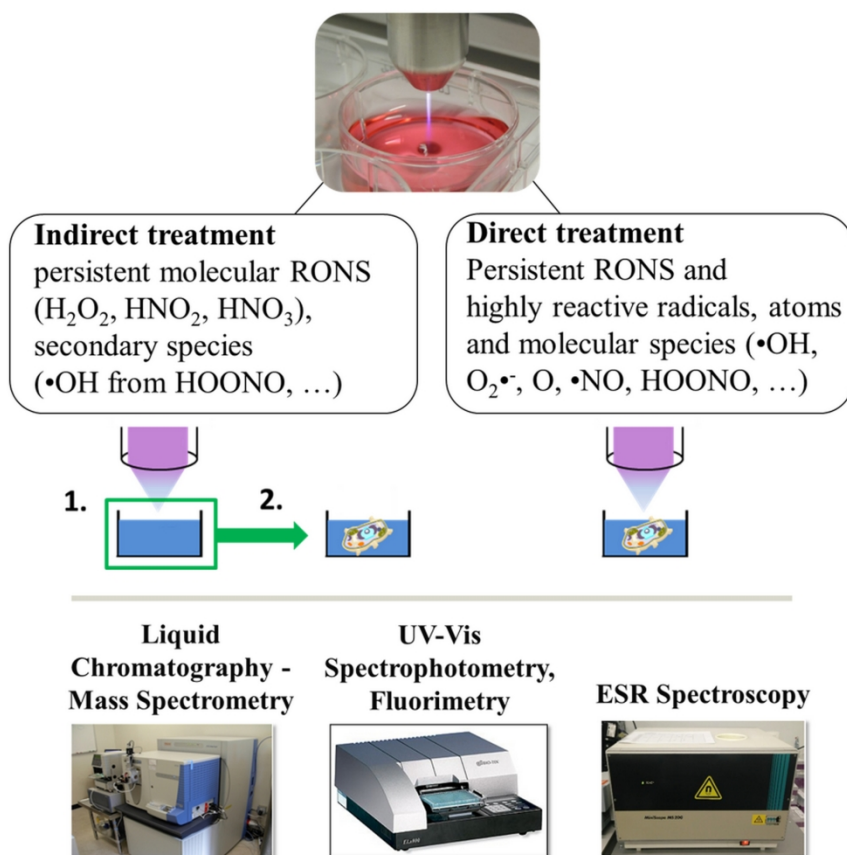


36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

Figure 2. Two methods of plasma application, RONS in solutions and main analytical techniques used for their detection.

354x329mm (150 x 150 DPI)

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

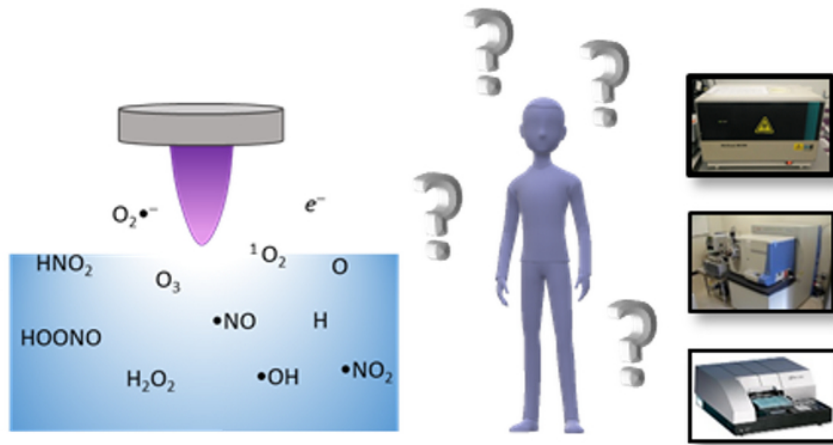

TOC graphic

141x102mm (150 x 150 DPI)